






FIG. 6

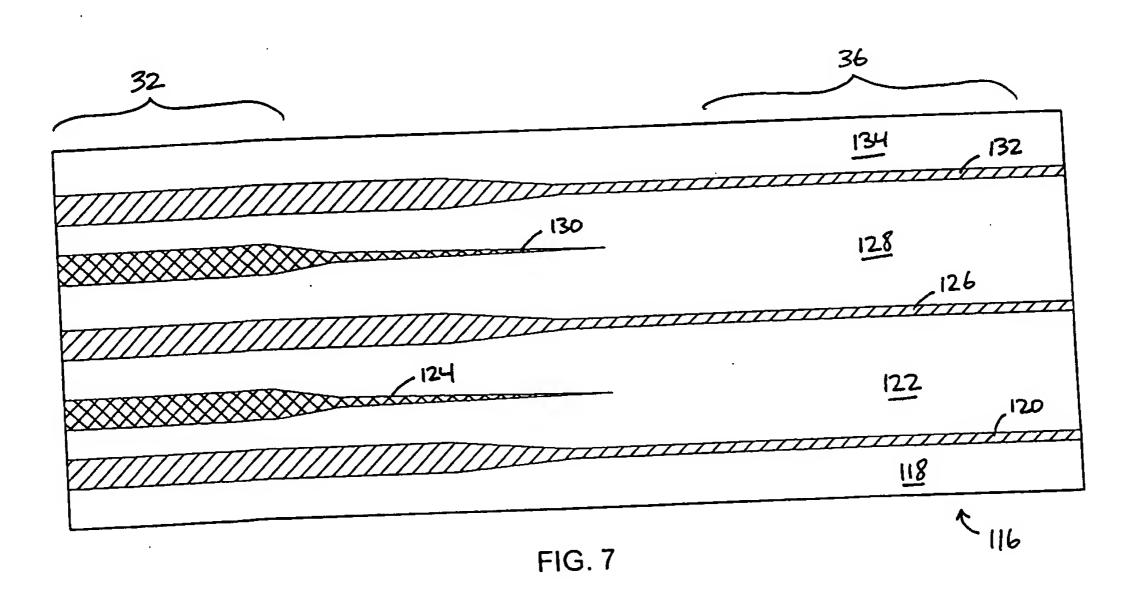

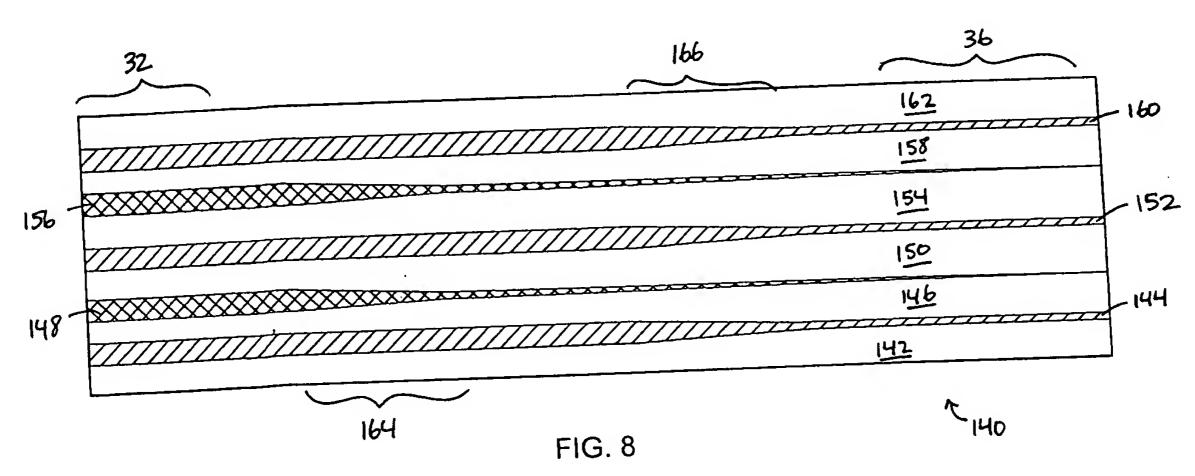


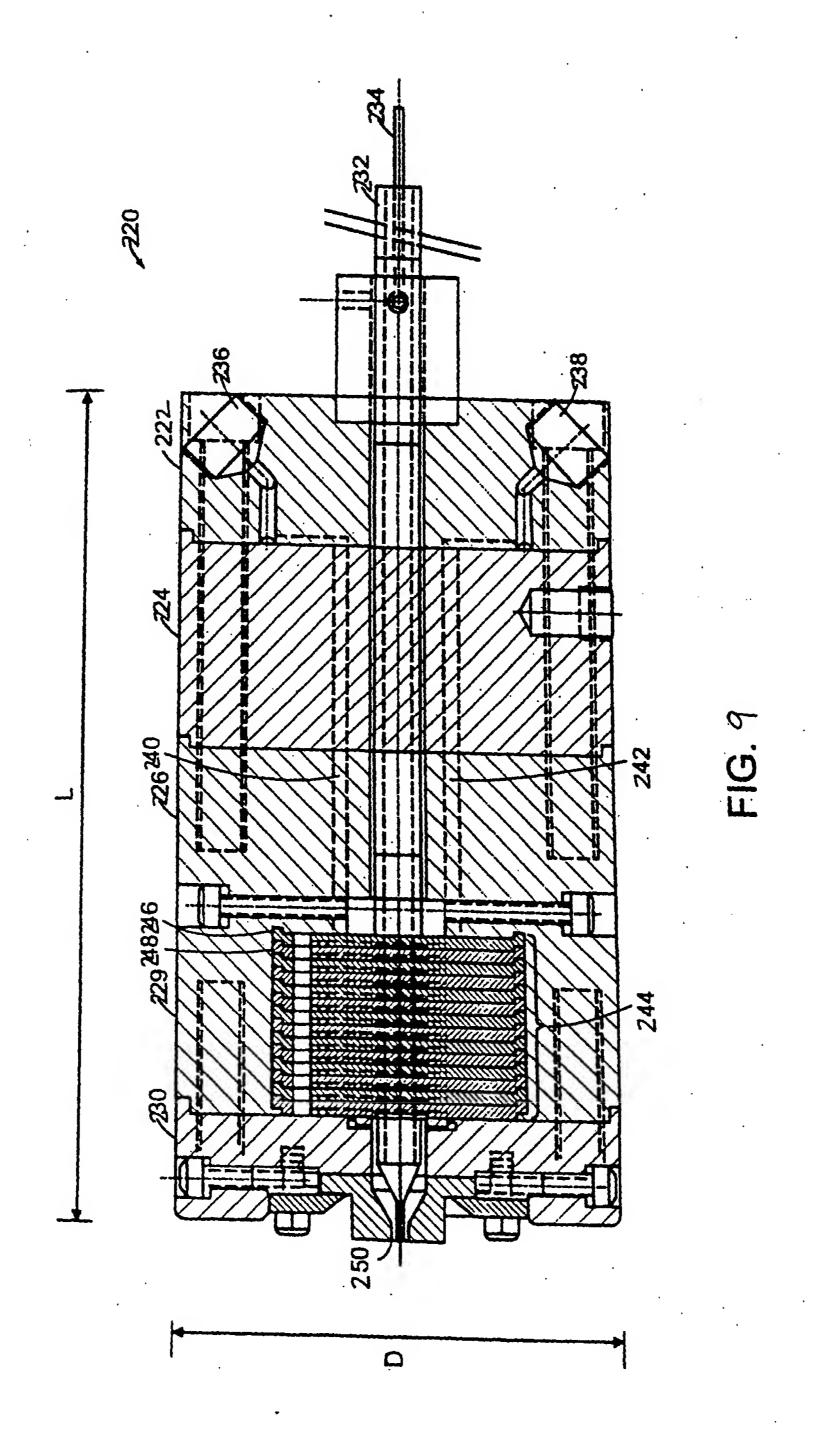


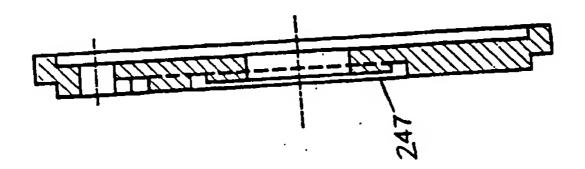

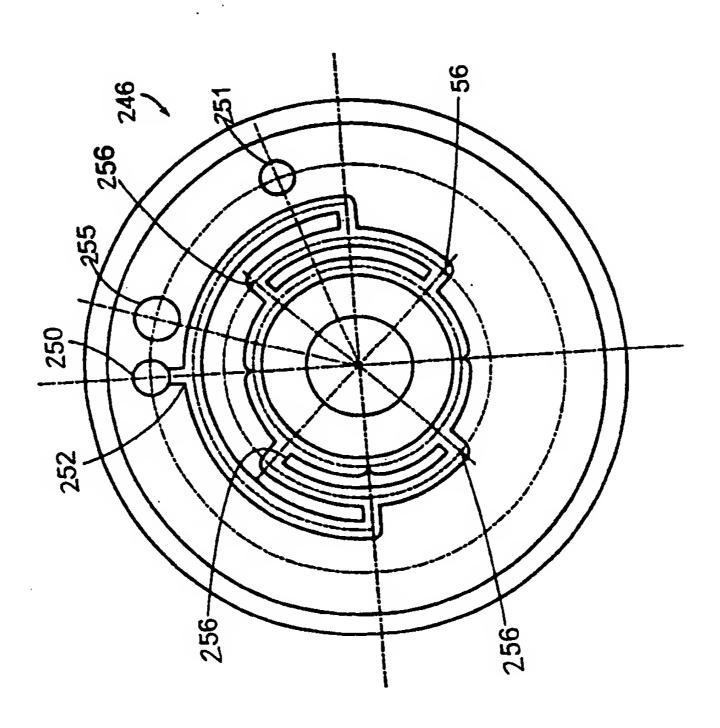



76. ga

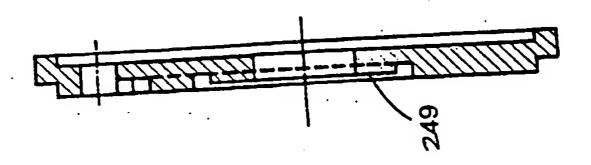


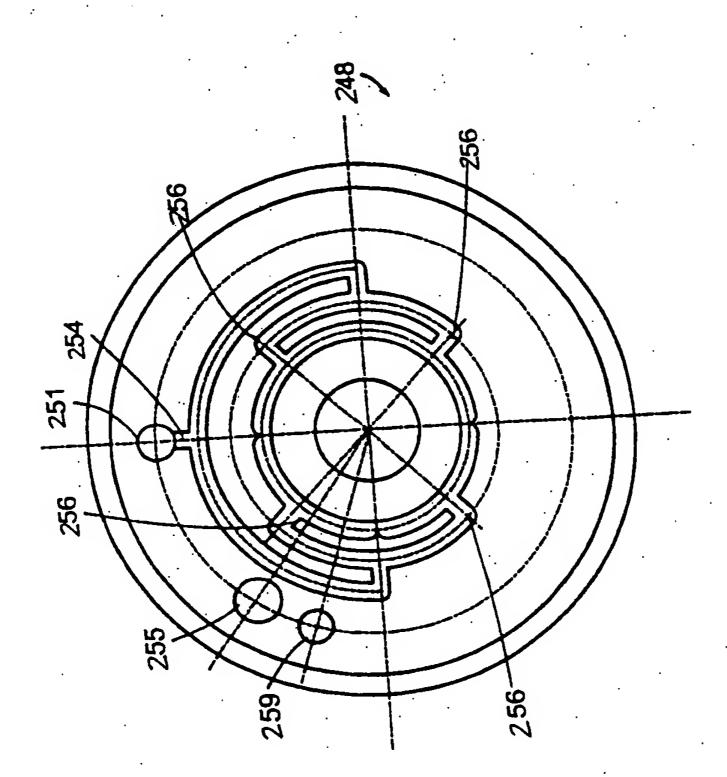



76.9b

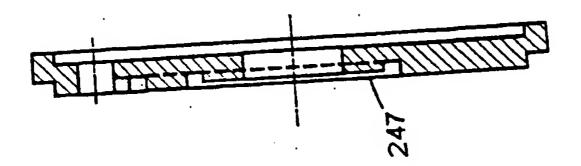



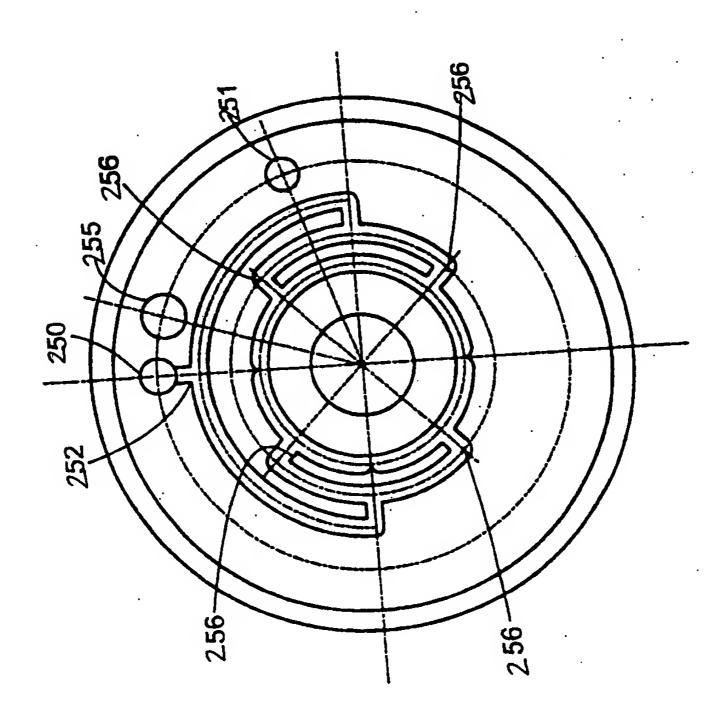


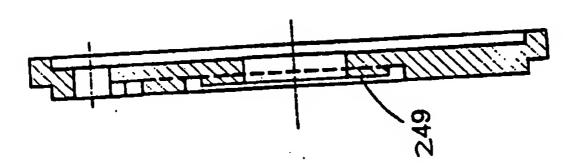

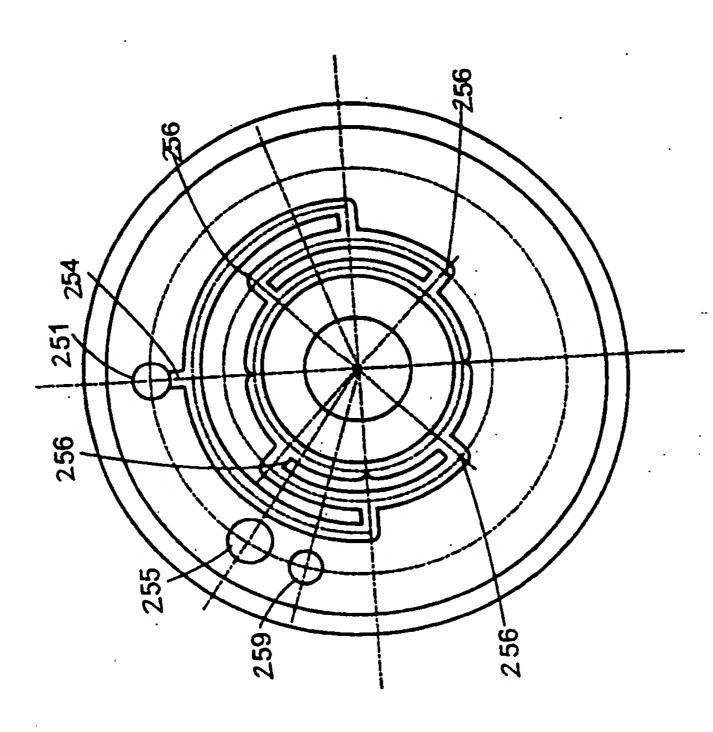

F. 9d

Page 9 of 22
MULTILAYER MEDICAL DEVICES
Douglas A. Devens, Jr.
10527-396001

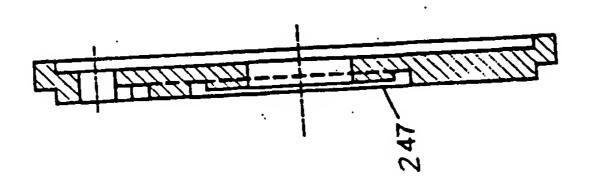

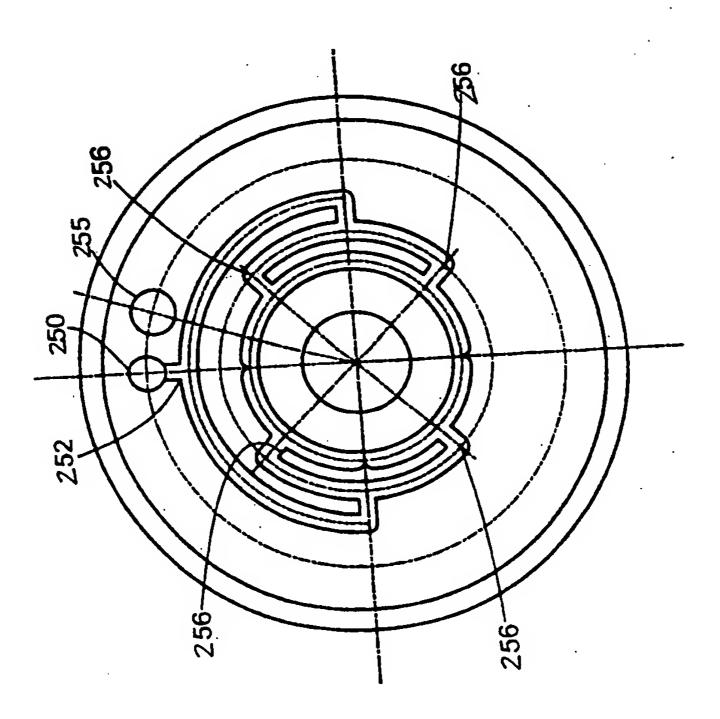


FIG. 9E

Page 10 of 22
MULTILAYER MEDICAL DEVICES
Douglas A. Devens, Jr.
10527-396001



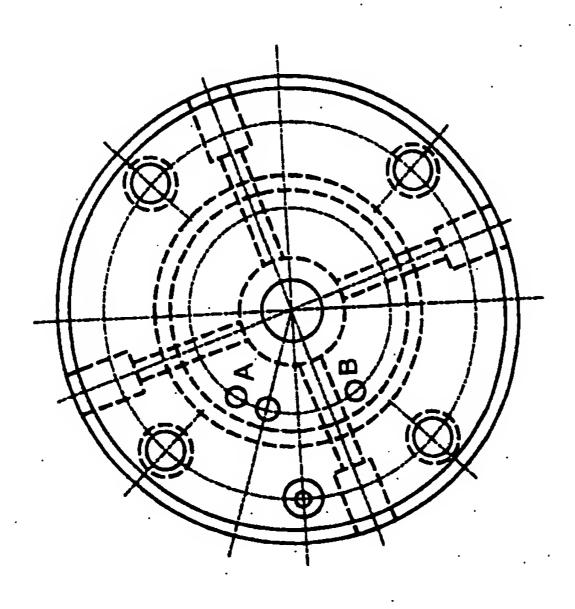


Fig. 9f

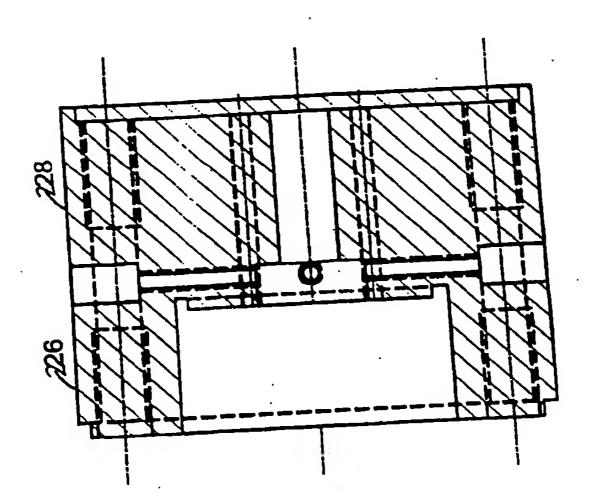



Page 11 of 22 MULTILAYER MEDICAL DEVICES Douglas A. Devens, Jr. 10527-396001

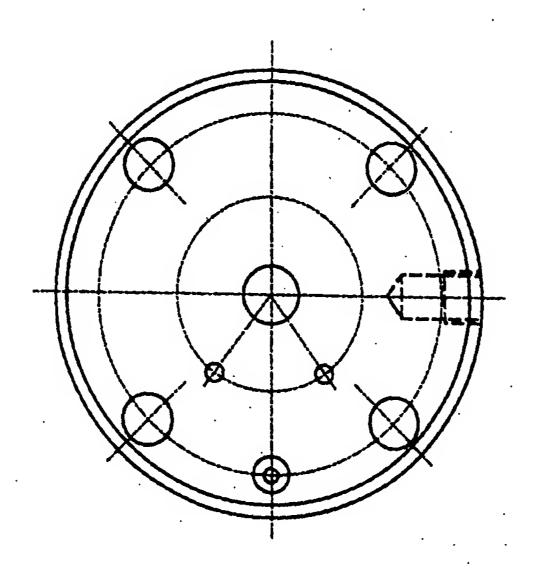



9


力の

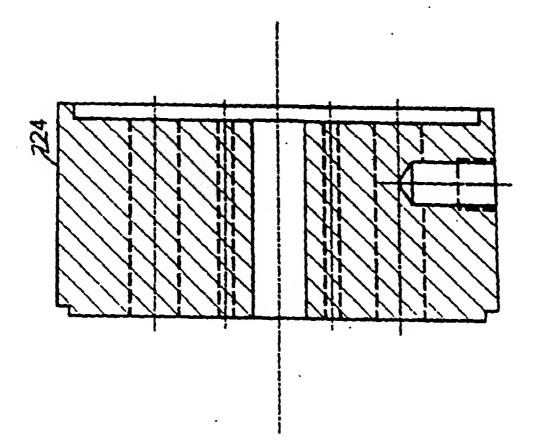

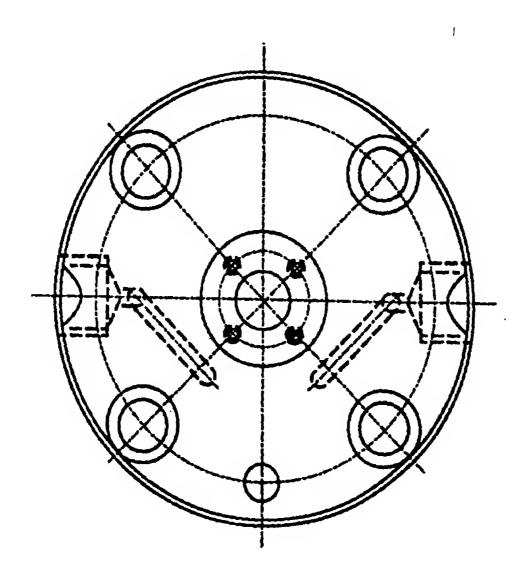


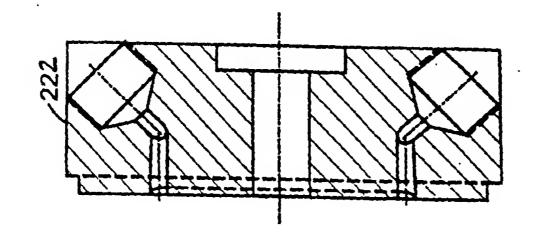




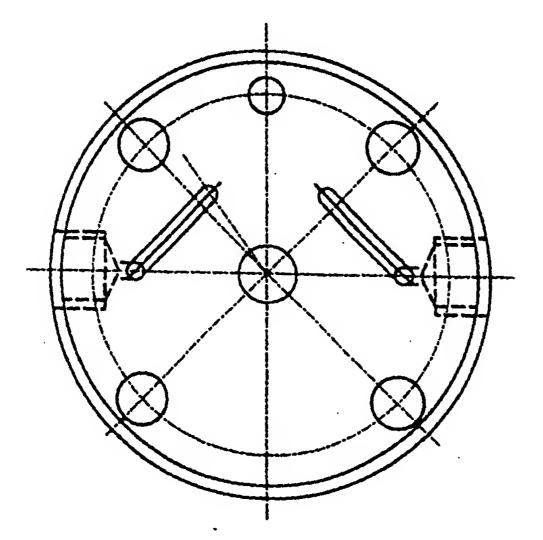


Page 13 of 22
MULTILAYER MEDICAL DEVICES
Douglas A. Devens, Jr.
10527-396001

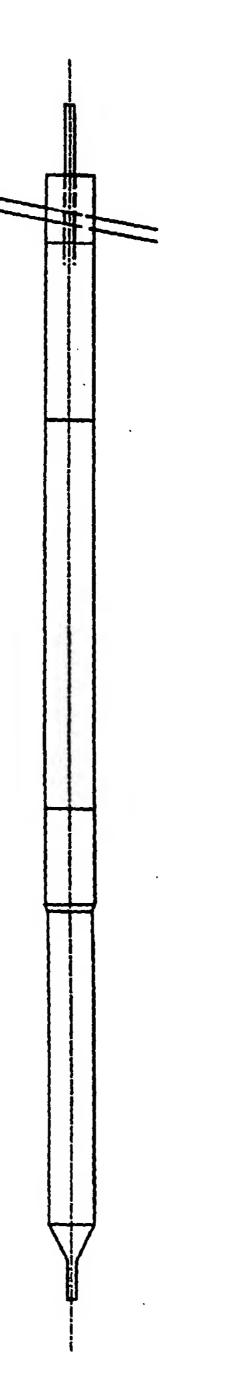


16.9%

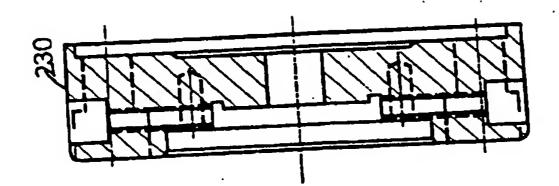

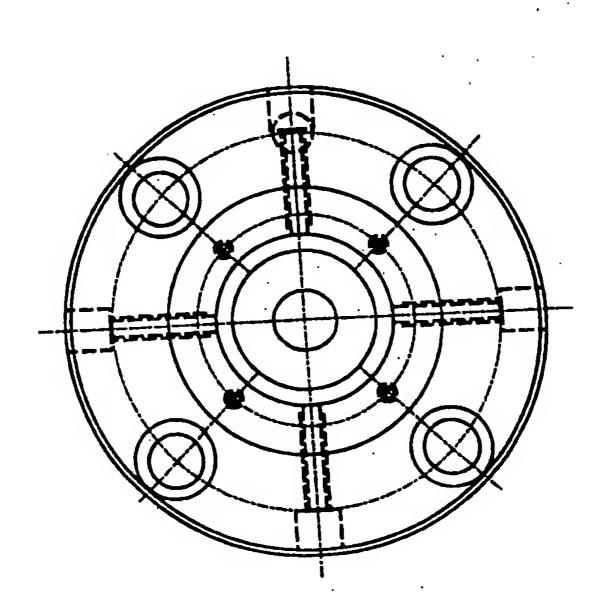


16. AJ


Page 15 of 22 MULTILAYER MEDICAL DEVICES Douglas A. Devens, Jr. 10527-396001



9K

五

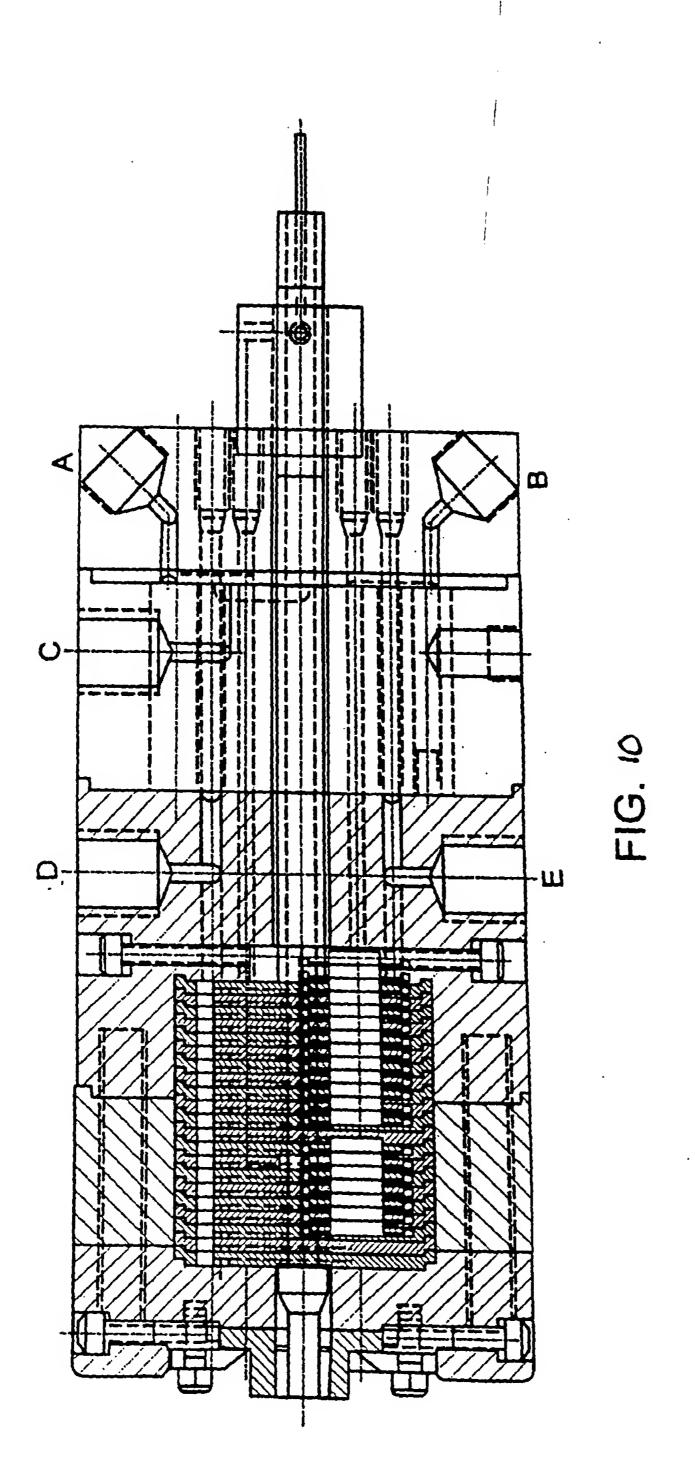

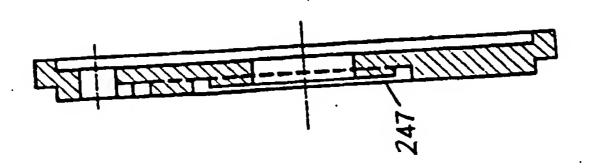



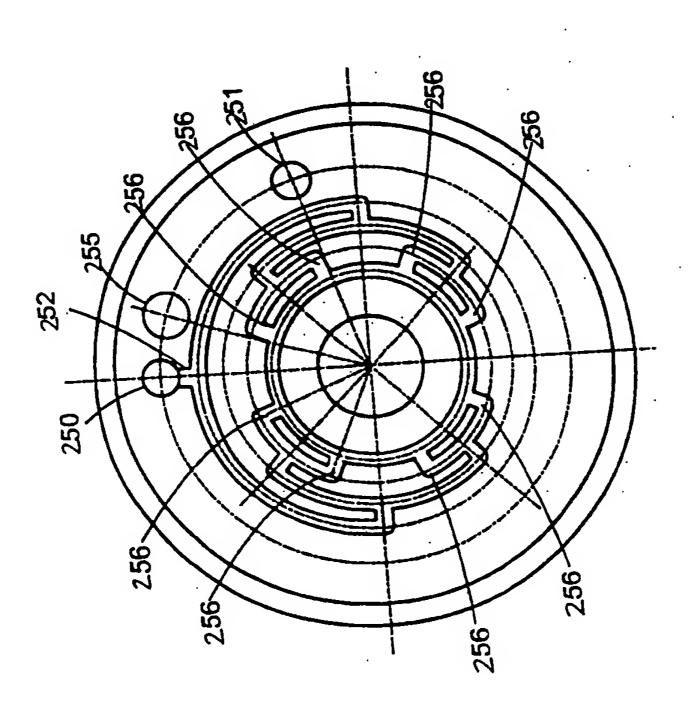



FIG. 11a

Page 18 of 22
MULTILAYER MEDICAL DEVICES
Douglas A. Devens, Jr.
10527-396001

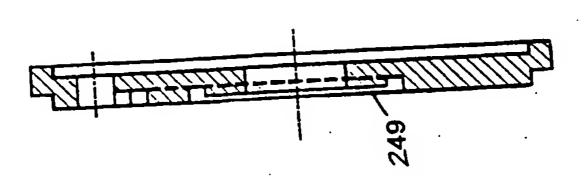


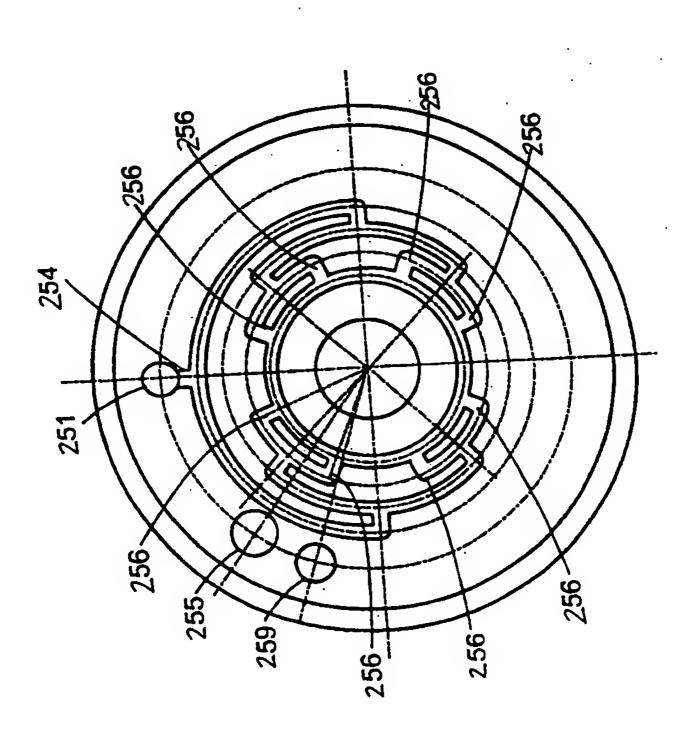



日の一日

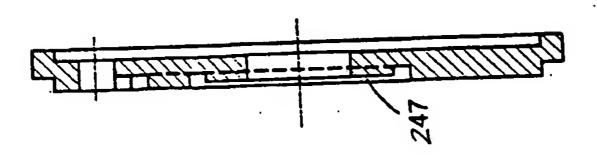



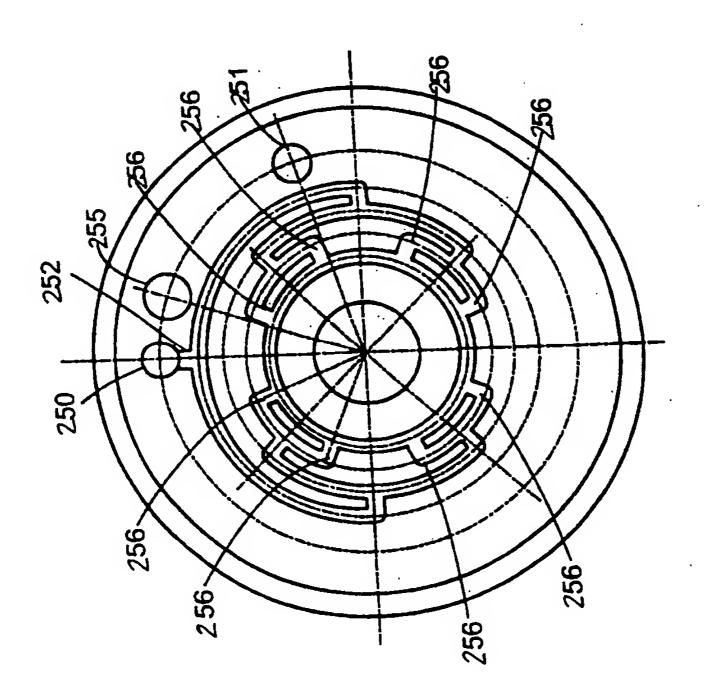


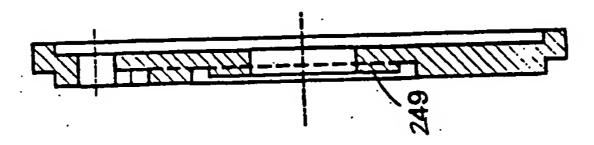


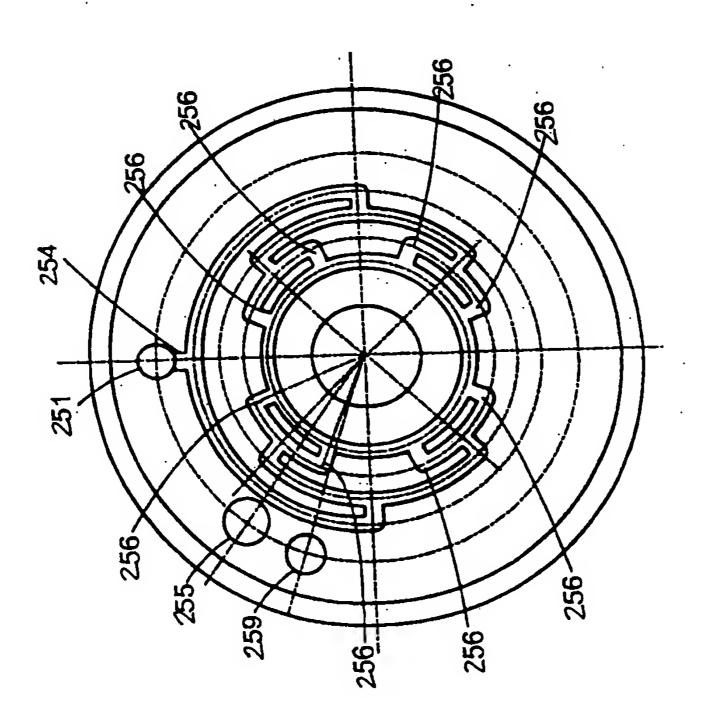

HG. 11 A

Page 21 of 22 MULTILAYER MEDICAL DEVICES Douglas A. Devens, Jr. 10527-396001

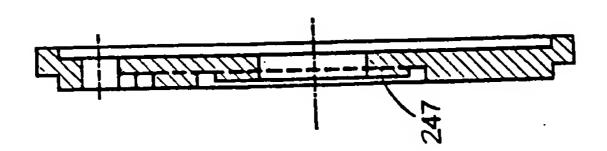

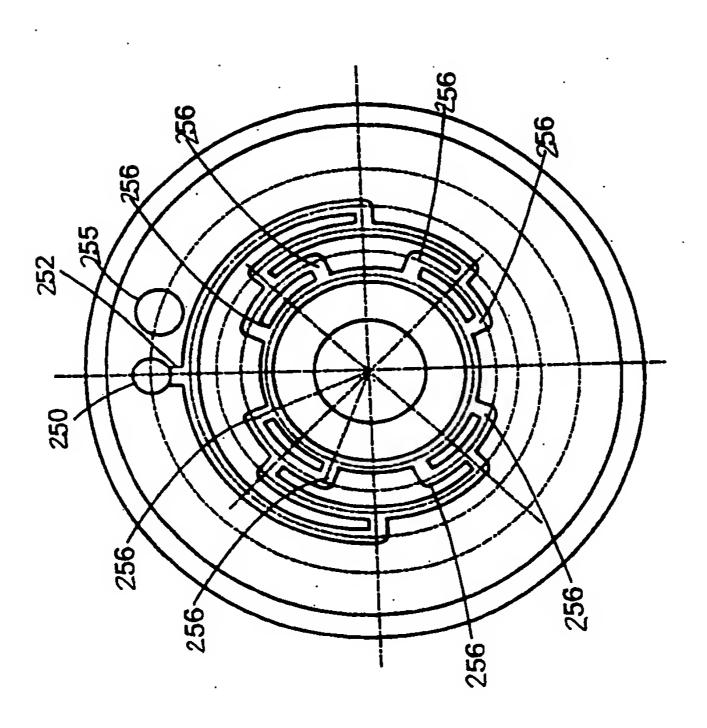

FG. 118

Page 22 of 22
MULTILAYER MEDICAL DEVICES
Douglas A. Devens, Jr.
10527-396001

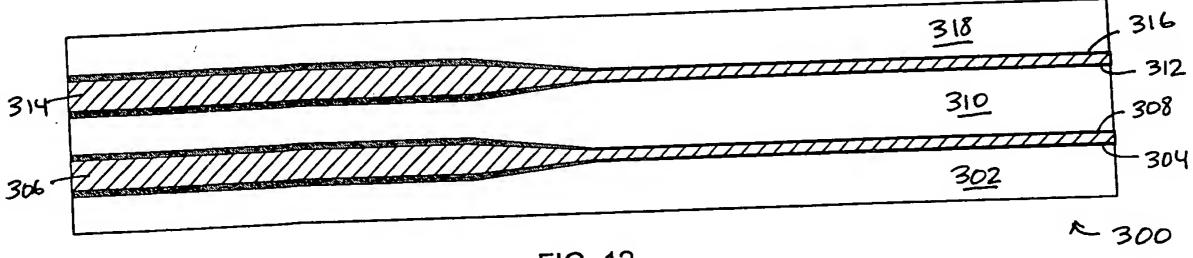


FIG. 12